



نتقدم بثقة
Moving Forward
with Confidence

رؤية عمان
2040
Oman Vision

To:

THE DIRECTOR GENERAL OF HEALTH SERVICES IN ALL GOVERNORATES
Commanding Officer, Armed Forces Hospital (Al Khoudh & Salalah)
Director General of Engineering Affairs, MOH
Director General of Royal Hospital
Director General of Khoula Hospital
Director General of Medical Supplies (MOH)
Director General of Pvt. Health Est. Affairs (to kindly arrange distribution to all Pvt. Hospitals)
Hospital Director (Al Nahda Hospital)
Hospital Director (Al Massara Hospital)
The Head of Medical Services in SQU Hospital
The Head of Medical Services in Royal Oman Police
The Head of Medical Services in Ministry of Defence
The Head of Medical Services in The Diwan
The Head of Medical Services in The Sultan's Special Force
The Head of Medical Services in Internal Security Services
The Head of Medical Services in Petroleum Development of Oman
The Head of Medical Services in LNG Oman
ALL PRIVATE PHARMACIES & DRUG STORES

After Compliments,

Please find attached our Circular No 38 dated 21/2/2023 Regarding NCMDR
FSCA of Silverline Cu 380 Ag from (mfr: Pregna International Ltd.).

Copy to:

- Director, Office of H.E. The Undersecretary for Health Affairs
- Director of Medical Device Control, DGPA&DC
- Director of Pharmacovigilance & Drug Information Dept, DGPA&DC
- Director of Drug Control Department, DGPA&DC
- Director of Pharmaceutical Licensing Department, DGPA&DC
- Director of Central Quality Control Lab., DGPA&DC
- Supdt. of Central Drug Information



Circular No. 38 / 2023

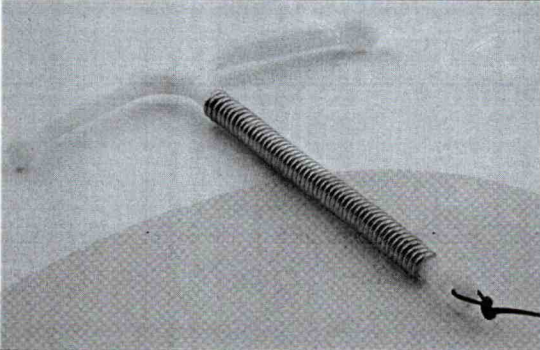
30 -07-1444 H

21 -02-2023

نتقدم بثقة
Moving Forward
with Confidence

رؤية عمان
2040
Oman Vision

Field Safety Corrective Action of Silverline Cu 380 Ag from Pregna International Ltd.

Source	NCMDR- National Center for Medical Devices Reporting- SFDA https://ncmdr.sfda.gov.sa/Secure/CA/CaViewRecall.aspx?caid=15&rid=18444
Product	Silverline Cu 380 Ag.
Description	Intrauterine Contraceptive Device.
Manufacturer	Pregna International Ltd.
The affected products	ALL
Reason	The current instructions for use "IFU" needs clarification in contraindication statements, and edits of spelling mistakes.
Action	1. Refer to amended IFU for Silverline Cu 380Ag. 2. Contact the local agent for remedial action.
Product Image	
comments	Healthcare professionals are encouraged to report any adverse events Suspected to be associated with the above device or any other medical device to Department of Medical Device Control through the E-mail: Med-device@moh.gov.om

Dr. Mohammed Hamdan Al Rubaie

Director General

