



To:

THE DIRECTOR GENERAL OF HEALTH SERVICES IN ALL GOVERNORATES

Commanding Officer, Armed Forces Hospital (Al Khoudh & Salalah)

Director General of Engineering Affairs, MOH

Director General of Royal Hospital

Director General of Khoula Hospital

Director General of Medical Supplies (MOH)

Director General of Pvt. Health Est. Affairs (to kindly arrange distribution to all Pvt. Hospitals)

Hospital Director (Al Nahda Hospital)

Hospital Director (Al Massara Hospital)

The Head of Medical Services in SQU Hospital

The Head of Medical Services in Royal Oman Police

The Head of Medical Services in Ministry of Defence

The Head of Medical Services in The Diwan

The Head of Medical Services in The Sultan's Special Force

The Head of Medical Services in Internal Security Services

The Head of Medical Services in Petroleum Development of Oman

The Head of Medical Services in LNG Oman

ALL PRIVATE PHARMACIES & DRUG STORES

After Compliments,

Please find attached our Circular No. 54..... dated 23/3/22 Regarding GHC recall of Stomach Tube from (mrf: Suzhou New Area Mingji Macromolecule Medical).

Copy to:

- Director, Office of H.E. The Undersecretary for Health Affairs
- Director of Medical Device Control, DGPA&DC
- Director of Pharmacovigilance & Drug Information Dept, DGPA&DC
- Director of Drug Control Department, DGPA&DC
- Director of Pharmaceutical Licensing Department, DGPA&DC
- Director of Central Quality Control Lab., DGPA&DC
- Supdt. of Central Drug Information




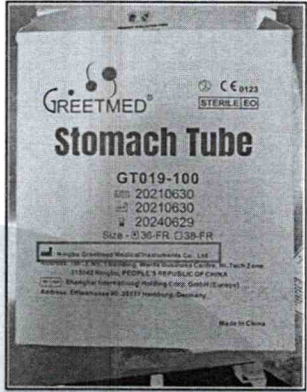
Circular No. 54/2022

20-08-1443 H

23-03-2022



Recall of Stomach Tube from Suzhou New Area Mingji Macromolecule Medical.

Source	GHC- Gulf Health Council.
Product	Stomach Tube.
Manufacturer	Suzhou New Area Mingji Macromolecule Medical.
The affected products	20210630.
Reason	Counterfeit medical devices.
Action	1. Discontinue using this device. 2. Contact the local agent for remedial action.
Product Picture	<div style="display: flex; justify-content: space-around; align-items: center;"> <div style="text-align: center;">  <p>Counterfeit device</p> </div> <div style="text-align: center;">  <p>Original Device</p> </div> </div>
comments	Healthcare professionals are encouraged to report any adverse events Suspected to be associated with the above device or any other medical device to Department of Medical Device Control contact E-mail: Med-device@moh.gov.om

AS
Dr. Mohammed Hamdan Al Rubaie
DIRECTOR GENERAL

